

Hysterosalpingosonography for diagnosing tubal occlusion in subfertile women: a systematic review with meta-analysis

S. Maheux-Lacroix^{1,2,*}, A. Boutin², L. Moore², M.-E. Bergeron^{1,2,3},
E. Bujold^{1,2}, P. Laberge^{1,2}, M. Lemyre^{1,2}, and S. Dodin^{1,2}

¹Department of Obstetrics, Gynecology and Reproduction, Université Laval, 2325, rue de l'Université, Québec, QC, Canada G1V 0A6 ²CHU de Québec Research Center, 2705, boul. Laurier, Québec, QC, Canada G1V 4G2 ³Oxford Fertility Unit, Institute of Reproductive Sciences, Nuffield Department of Obstetrics and Gynaecology, University of Oxford, Oxford OX4 2HW, UK

* Correspondence address. E-mail: sarah.maheux.lacroix@gmail.com

Submitted on September 23, 2004; resubmitted on January 15, 2014; accepted on January 23, 2014

STUDY QUESTION: Is hysterosalpingosonography (sono-HSG) an accurate test for diagnosing tubal occlusion in subfertile women and how does it perform compared with hysterosalpingography (HSG)?

SUMMARY ANSWER: sono-HSG is an accurate test for diagnosing tubal occlusion and performs similarly to HSG.

WHAT IS KNOWN ALREADY: sono-HSG and HSG are both short, well-tolerated outpatient procedures. However, sono-HSG has the advantage over HSG of obviating ionizing radiation and the risk of iodine allergy, being associated with a greater sensitivity and specificity in detecting anomalies of the uterine cavity and permitting concomitant visualization of the ovaries and myometrium.

STUDY DESIGN, SIZE, DURATION: A systematic review and meta-analysis of studies published in any language before 14 November 2012 were performed. All studies assessing the accuracy of sono-HSG for diagnosing tubal occlusion in a subfertile female population were considered.

PARTICIPANTS/MATERIALS, SETTING, METHODS: We searched Medline, Embase, Cochrane Library, Web of Science and Biosis as well as related articles, citations and reference lists. Diagnostic studies were eligible if they compared sono-HSG (\pm HSG) to laparoscopy with chromotubation in women suffering from subfertility. Two authors independently screened for eligibility, extracted data and assessed the quality of included studies. Risk of bias and applicability concerns were investigated according to the Quality Assessment of Diagnostic Accuracy Study (QUADAS-2). Bivariate random-effects models were used to estimate pooled sensitivity and specificity with their 95% confidence intervals (95% CIs), to generate summary receiver operating characteristic curves and to evaluate sources of heterogeneity.

MAIN RESULTS AND THE ROLE OF CHANCE: Of the 4221 citations identified, 30 studies were eligible. Of the latter, 28 reported results per individual tube and were included in the meta-analysis, representing a total of 1551 women and 2740 tubes. In nine studies, all participants underwent HSG in addition to sono-HSG and laparoscopy, allowing direct comparison of the accuracy of sono-HSG and HSG. Pooled estimates of sensitivity and specificity of sono-HSG were 0.92 (95% CI: 0.82–0.96) and 0.95 (95% CI: 0.90–0.97), respectively. In nine studies (582 women, 1055 tubes), sono-HSG and HSG were both compared with laparoscopy, giving pooled estimates of sensitivity and specificity of 0.95 (95% CI: 0.78–0.99) and 0.93 (95% CI: 0.89–0.96) for sono-HSG, and 0.94 (95% CI: 0.74–0.99) and 0.92 (95% CI: 0.87–0.95) for HSG, respectively. Doppler sonography was associated with significantly greater sensitivity and specificity of sono-HSG compared with its non-use (0.93 and 0.95 versus 0.86 and 0.89, respectively, $P = 0.0497$). Sensitivity analysis regarding methodological quality of studies was consistent with these findings. We also found no benefit of the commercially available contrast media over saline solution in regard to the diagnostic accuracy of sono-HSG.

LIMITATIONS, REASONS FOR CAUTION: Methodological quality varied greatly between studies. However, sensitivity analysis, taking methodological quality of studies into account, did not modify the results. This systematic review did not allow the distinction between distal and proximal occlusion. This could be interesting to take into account in further studies, as the performance of the test may differ for each localization.

WIDER IMPLICATIONS OF THE FINDINGS: Given our findings and the known benefits of sono-HSG over HSG in the context of subfertility, sono-HSG should replace HSG in the initial workup of subfertile couples.

STUDY FUNDING/COMPETING INTEREST(S): This study was funded by personal funds. There are no conflicts of interest to declare.

TRIAL REGISTRATION NUMBER: This review has been registered at PROSPERO: Registration number #CRD42013003829.

Key words: hysterosalpingosonography / hysterosalpingography / diagnostic / tubal patency / systematic review

Introduction

Hysterosalpingosonography (sono-HSG), an ultrasound-based technique, has been proposed as an alternative to hysterosalpingography (HSG) to assess tubal patency in the initial workup of subfertile couples (NICE, 2013). Sono-HSG and HSG are both short, well-tolerated outpatient procedures (Dessole et al., 2003; Savelli et al., 2009; Socolov et al., 2010). However, sono-HSG has the advantage of obviating ionizing radiation and the risk of iodine allergy associated with HSG (Saunders et al., 2011). Compared with HSG, sono-HSG also has greater sensitivity and specificity in detecting anomalies of the uterine cavity (Soares et al., 2000; Acholonu et al., 2011) and permits concomitant visualization of the ovaries and myometrium (Saunders et al., 2011).

Both sono-HSG and HSG are substitutes for laparoscopy, which is largely accepted as the gold standard for diagnosing tubal occlusion (Mol et al., 1999; Saunders et al., 2011; NICE, 2013). However, being a more costly and invasive test (Saunders et al., 2011), laparoscopy is usually indicated for women who could also benefit from a laparoscopy for the assessment or treatment of another pelvic pathology (NICE, 2013).

A systematic review with meta-analysis comparing sono-HSG and HSG to laparoscopy for diagnosing tubal occlusion was published in Holz et al. (1997). In this review, sono-HSG was associated with a 10% rate of false occlusion and 7% of false patency compared with 13 and 11%, respectively, with HSG. Since then, several reports have been published (Saunders et al., 2011) and the techniques implemented for sono-HSG have greatly improved with the arrival of new contrast media, three-dimensional (3D) ultrasonography, colour-coded 3D power Doppler imaging and heightened ultrasound resolution (Kiyokawa et al., 2000; Sladkevicius et al., 2000; Sankpal et al., 2001).

Our primary objective was to determine the diagnostic accuracy of sono-HSG for detecting tubal occlusion in women suffering from subfertility. Our secondary objective was to compare the diagnostic accuracy of sono-HSG and HSG. We planned to investigate sources of heterogeneity, namely differences in sono-HSG techniques and methodological quality of the included studies.

Materials and Methods

Design

The design of this systematic review was elaborated by a multidisciplinary group of experts (in reproductive endocrinology and infertility, ultrasound in obstetrics and gynaecology, minimally invasive gynaecology and research methodologies) according to approaches outlined in the 'Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy' (Deeks et al., 2008). This article was written in accordance with 'Preferred Reporting Items for Systematic Reviews and Meta-Analyses' (PRISMA) (Liberati et al., 2009). Our protocol was registered with PROSPERO (#CRD42013003829) and published *a priori* (Maheux-Lacroix et al., 2013).

Search strategy

We searched Medline, Embase, Cochrane Library and the Web of Science from their inception to 14 November 2012. Biosis was used to identify relevant abstracts and conference proceedings. The search strategy for Medline is presented in Supplementary data, Fig. S1. As recommended in the literature (Leefflang et al., 2006; de Vet et al., 2008; Reitsma et al., 2012), we developed a search strategy with terms related to the index test (sono-HSG) and the target condition (tubal occlusion) and did not use any filter for diagnostic studies to maximize the sensitivity of the search. The strategy was revised by a healthcare librarian and all authors. Finally, we looked at reference lists and citations of relevant articles (previous reviews and included studies) to identify additional eligible reports.

Eligibility criteria and study selection

We considered all studies assessing the accuracy of sono-HSG for diagnosing tubal occlusion in a subfertile female population. There were no restrictions in terms of publication date or language. Articles written in languages other than English or French were translated before completing the selection process and data abstraction. Studies including women suffering from recurrent spontaneous miscarriages were eligible. We excluded studies that undertook sono-HSG to confirm occlusion after tubal sterilization, these samples being significantly different from the population of interest.

We only considered studies using exclusively laparoscopy as reference standard. Studies considering other modalities as reference standard, such as HSG, hysteroscopic selective tubal cannulation under fluoroscopic guidance or vaginal laparoscopy, were excluded. For studies using HSG as a comparator test (that is, additionally assessing the accuracy of HSG compared with laparoscopy), data on the diagnostic accuracy of HSG was retained in order to make a direct comparison of accuracy between sono-HSG and HSG.

We considered consecutive and random series of patients as well as case-control designs.

Studies utilizing random partial verification and non-random partial verification were eligible, provided the determinants of partial verification were known and verification in each strata was random and in known proportions (Irwig et al., 1994; de Groot et al., 2011; de Groot et al., 2012).

Study eligibility was assessed independently by two reviewers screening titles, abstracts and full-text publications, when required. If disagreements were not resolved by consensus, a third reviewer was consulted. Attempts were made to contact the author for further information on studies that fulfilled the eligibility criteria but did not have sufficient data to build 2-by-2 tables. We collected reasons for full-text exclusion. To avoid duplication, author names, sample sizes and study results were compared.

Data abstraction

Two authors independently extracted data from included studies, and disagreements were resolved by discussion. If consensus was not reached, a third reviewer was consulted. We developed a standardized data abstraction form, which was pilot-tested on three studies (Spalding et al., 1997; Inki et al., 1998; Reis et al., 1998) and refined accordingly. The following information was extracted from each of them:

- (1) Study characteristics and methods: study design, inclusion and exclusion criteria, flow diagram, setting, country, language of publication.

- (2) Description of the sono-HSG technique: resolution, two-dimensional (2D) or 3D device, vaginal or abdominal probe, contrast type, catheter type and Doppler sonography.
- (3) Measures of diagnostic accuracy of sono-HSG (and HSG when available) in reference to laparoscopy.

In some studies, a positive test was defined as the presence of an occluded tube and, in others, by the presence of a patent tube. In order to pool the results, we reported the data of all studies by considering a positive test as an occluded tube. If published data did not allow us to obtain or derive the number of true positives (TP), false positives (FP), true negatives (TN) and false negatives (FN), we attempted to contact the corresponding author of the study.

Assessment of methodological quality

Two persons independently assessed the risk of bias and applicability concerns with a quality checklist derived from the Quality Assessment of Diagnostic Accuracy Study (QUADAS-2; Whiting *et al.*, 2011) and available in our published protocol (Maheux-Lacroix *et al.*, 2013). In case of discrepancy, a third reviewer was consulted. An interval of no more than 1 month between tests was considered appropriate. Sono-HSG (\pm HSG) results had to be interpreted without knowledge of the laparoscopy results. Reviewers' judgements about risks of bias and applicability concerns were used in sensitivity analysis to examine the effect of methodological quality of studies.

Statistical analysis and data synthesis

Meta-analysis was performed by computing the number of TP, TN, FP and FN of each study in bivariate hierarchical random-effects models using SAS 9.3 (SAS Institute, Inc., Cary, NC, USA, 2011). The results were presented with Cochrane Review Manager version 5.2 (The Nordic Cochrane Centre, The Cochrane Collaboration, Copenhagen, Denmark, 2012).

Pooled and individual estimates of sensitivity and specificity and 95% confidence intervals (95% CIs) were presented in paired forest plots. We generated summary receiver operating characteristic (SROC) curves with point estimates for each study as well as symmetrical summary curves, summary point estimates, 95% confidence region and 95% prediction region. The magnitude of heterogeneity was assessed with the 95% prediction region on SROC curves.

Direct comparison of sono-HSG and HSG accuracy as well as subgroup and sensitivity analyses were achieved using bivariate models. We *a priori* planned to examine the effect of differences in sono-HSG technique [2D versus 3D, low (<5 MHz) versus high resolution (\geq 5 MHz), Doppler versus standard sonography, vaginal versus abdominal probe, saline versus other contrast and flexible versus rigid catheter] and in the methodological quality of studies (low versus high or unclear global risks of bias and applicability concerns). We calculated *P*-values ($\alpha < 0.05$ was considered statistically significant) by computing the change in the -2 Log likelihood when the covariate was added to the model using the χ^2 statistic.

Results

Search results

We identified 4221 citations, with 160 studies that were considered potentially eligible for our systematic review after screening titles and abstracts (Fig. 1). One hundred and twenty-six studies were excluded because they did not meet the inclusion criteria. Four additional studies were excluded because we did not have sufficient data to build 2-by-2 tables and attempts to contact the authors failed. At the end of this process, a total of 30 studies were included in the systematic

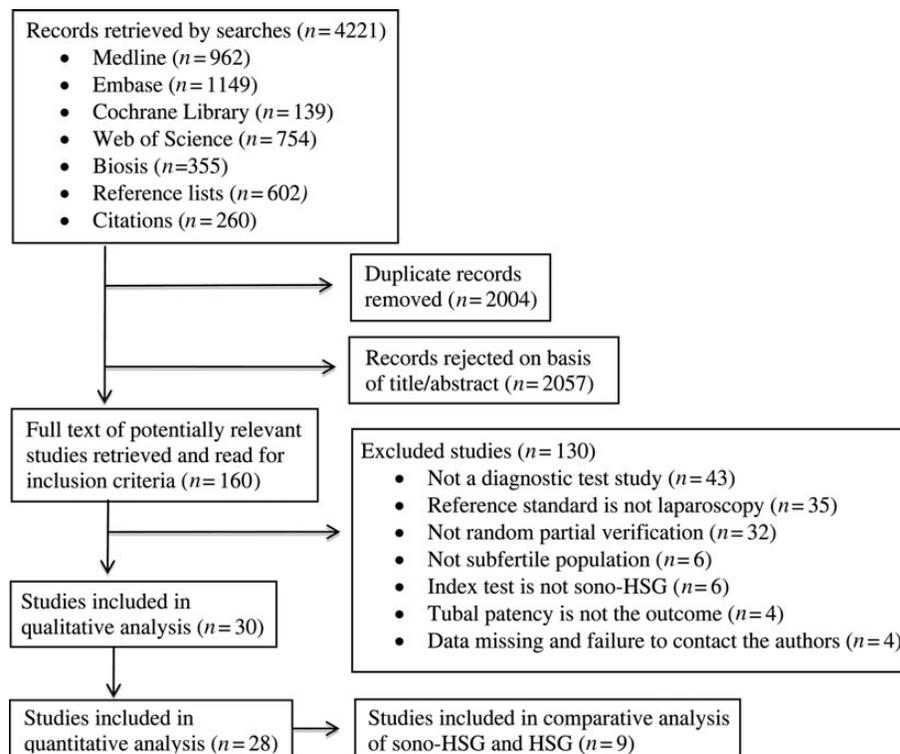


Figure 1 Search results for a systematic review of the accuracy of sono-HSG for diagnosing tubal occlusion in subfertile women.

review. Of them, 28 reported their results per tube and were considered in the meta-analyses. In nine studies, all participants underwent HSG in addition to sono-HSG and laparoscopy, allowing direct comparison of sono-HSG and HSG accuracies (Table I).

Study characteristics

Table I summarizes the characteristics of the included studies. All of them were published in peer-reviewed journals between 1986 and 2012. Studies were from North and South America, Europe, Asia and Africa, and six were not published in English. The prevalence of tubal occlusion varied from 7 to 89% across studies. Sono-HSGs were performed with a vaginal probe of 5 MHz or more and a flexible balloon catheter (5–10 French) in 24 studies, with an abdominal probe (<5 MHz) and rigid catheter in four studies and with either mode in two studies. The contrast agent was saline solution in 13 studies, galactose solution (Echovist, Schering AG, Berlin, Germany) in 15 studies and sulphur hexafluoride solution (SonoVue, Bracco, Milan, Italy) in one study. Thirteen studies reported using Doppler technology, and in five studies a 3D device was used.

Accuracy of sono-HSG for diagnosing tubal occlusion

Twenty-eight studies, representing 1551 women and 2740 tubes, served to estimate the global accuracy of sono-HSG for diagnosing tubal occlusion. Pooled estimates of sensitivity and specificity were 0.92 (95% CI: 0.82–0.96) and 0.95 (95% CI: 0.90–0.97), respectively. Paired forest plots and the corresponding SROC curve are presented in Fig. 2. The large prediction region on the SROC curve reflects heterogeneity between studies.

Two studies (Randolph et al., 1986; de Almeida et al., 2000) were excluded from the meta-analysis because they did not report results per individual tube. The study by de Almeida et al. (2000) ($n = 30$ women) achieved sensitivity and specificity of 1.00 (95% CI: 0.40–1.00) and 0.91 (95% CI: 0.80–0.97), respectively, for the detection of bilateral obstruction, and Randolph et al. (1986) study ($n = 61$ women) reached a specificity of 0.92 (95% CI: 0.74–0.99) for the detection of at least one occluded tube (TP number was unknown, which prevented the calculation of sensitivity).

Direct comparison of sono-HSG and HSG for diagnosing tubal occlusion

Sono-HSG and HSG were directly compared with laparoscopy by chromotubation in nine studies, representing 582 women and 1055 tubes. Figure 3 presents individual and pooled estimates of diagnostic accuracy parameters of both tests and SROC curves. For sono-HSG, pooled estimates of sensitivity and specificity were 0.95 (95% CI: 0.78–0.99) and 0.93 (95% CI: 0.89–0.96), respectively. For HSG, pooled estimates of sensitivity and specificity were 0.94 (95% CI: 0.74–0.99) and 0.92 (95% CI: 0.87–0.95), respectively. Differences between the two techniques were not statistically significant with a P -value of 0.4.

Methodological quality of studies

Figure 4 summarizes the risks of bias and applicability concerns of studies based on QUADAS-2 (the assessment of each individual study is presented in Supplementary data, Fig. S2). Only six studies specified that they presented consecutive series of patients (low risk of bias in terms

of patient selection). Most studies ($n = 19$) reported a clear definition of a positive test and how they ensured adequate blinding (low risk of bias in terms of 'index test'). In terms of 'flow and timing', 10 studies were considered a high risk of bias either because an interval of more than 1 month separated the tests or more than 10% of tubes were excluded from the final analysis. Reasons reported for exclusions were: poor visualization, cervical stenosis, pain, suspicion of hydrosalpinx at sonography (sono-HSG cancelled), pregnancy and the women failed to return for the other test. All included studies had a complete verification design (gold standard performed on all participants; low risk of bias in terms of reference standard). Applicability concerns were raised in 11 studies that either exclusively recruited subfertile women with planned laparoscopy, included women suffering from recurrent pregnancy loss or undertook sono-HSG under general anaesthesia just before laparoscopy (applicability concerns in terms of 'patient selection'). In summary, 14 studies were considered a high risk of bias or raised applicability concerns for at least one item of the QUADAS-2 tool.

Subgroup and sensitivity analyses

Subgroup and sensitivity analyses are presented in Table II. Doppler sonography for sono-HSG was associated with significantly higher sensitivity and specificity compared with its non-use (0.93 and 0.95 versus 0.86 and 0.89, respectively, $P = 0.0497$). Estimates were not statistically different when comparing 3D with 2D and saline with other contrasts. Data available for the estimation of pooled sensitivity and specificity with abdominal probes, low-resolution devices (<5 MHz), and rigid catheters came from only four studies (Allahbadia et al., 1992; Omigbodun et al., 1992; Allahbadia, 1993; Kozarzewski et al., 1995) of unclear methodological quality (3/7 to 5/7 items on QUADAS-2 were unclear); therefore, these subgroup analyses were not performed.

Analysis based on global score of risk of bias and applicability concerns revealed that the methodological quality of the studies did not modify pooled estimates of sono-HSG sensitivity or specificity ($P = 0.5$).

Discussion

In this systematic review, we observed high diagnostic accuracy of sono-HSG for tubal occlusion with overall sensitivity of 0.92 (95% CI: 0.82–0.96) and specificity of 0.95 (95% CI: 0.90–0.97). We also found that the diagnostic accuracy of sono-HSG and HSG was comparable with no significant difference in performance of the two tests.

Sono-HSG presents some advantages over HSG. First, sono-HSG avoids the risk of allergy and ionizing radiation associated with iodinate contrast and fluoroscopic guidance of HSG. Secondly, sono-HSG was associated with greater sensitivity and specificity for the detection of intrauterine pathologies, such as fibromas, polyps and synechiae in subfertile populations (Soares et al., 2000; Acholonu et al., 2011). Finally, unlike HSG, sono-HSG permits concomitant visualization of the ovaries and myometrium, which can result in relevant findings in a context of subfertility, such as polycystic ovaries, endometriomas, other ovarian cysts and Müllerian anomalies (Saunders et al., 2011).

Sono-HSG and HSG are both short and well-tolerated outpatient procedures (Ayida et al., 1996; Dessole et al., 2003; Savelli et al., 2009; Lim et al., 2011). In a series of 1153 sono-HSG (Dessole et al., 2003), adverse effects occurred in only 8.8% of cases (moderate or severe pelvic pain 3.8%, vasovagal symptoms 3.5%, nausea 1.0%, vomiting 0.5% and

Table 1 Characteristics of included studies in a systematic review of the accuracy of sono-HSG for diagnosing tubal occlusion in subfertile women.

Studies	Participants	Tubes ^a (excluded)	Country	Language	Population	Prevalence ^b	Contrast	Catheter	Resolution (MHz)	Probe	2D or 3D	Doppler	Comparison with HSG ²	In MA
Allahbadia (1992)	129	129 (0)	India	English	Subfertility	0.11	Saline + air	Flexible with balloon (8 Fr) or rigid	3.5–5	Vaginal or abdominal	2D	Yes	Yes	Yes
Allahbadia (1993)	27	54 (0)	India	English	Subfertility	0.22	Saline	Rigid	2.5	Abdominal	2D	Yes	Yes	Yes
Allahbadia (1994)	53	106 (0)	India	English	Subfertility	0.11	Saline	Rigid or flexible with balloon (8 Fr)	2.5–5	Vaginal or abdominal	2D	Yes	Yes	Yes
Allahbadia <i>et al.</i> (1992)	50	100 (0)	India	English	Subfertility	0.15	Saline + air	Flexible with balloon (8 Fr)	5	Vaginal	2D	Yes	Yes	Yes
Ayida <i>et al.</i> (1997)	20	32 (7)	England	English	Subfertility with planned laparoscopy	0.12	Galactose	Flexible with balloon (5–7 Fr)	5–6	Vaginal	2D	No	No	Yes
Battaglia <i>et al.</i> (1996)	59	114 (4)	Italy	English	Subfertility	0.17	Saline	Flexible with balloon	5–6.5	Vaginal	2D	Yes	Yes	Yes
Chan <i>et al.</i> (2005)	21	34 (8)	China	English	Subfertility with planned laparoscopy	0.26	Galactose	Flexible with balloon (8 Fr)	7	Vaginal	3D	Yes	No	Yes
de Almeida <i>et al.</i> (2000)	30	60 (8)	Brazil	Portuguese	Subfertility	0.04	Galactose	Flexible with balloon (10 Fr)	5	Vaginal	2D	No	Yes	No
De Jonge <i>et al.</i> (2001)	100	178 (22)	South Africa	English	Primary subfertility	0.89	Galactose	Flexible with balloon (5 Fr)	6	Vaginal	2D	No	No	Yes
Dietrich <i>et al.</i> (1996)	20	39 (1)	Germany	English	Subfertility	0.13	Saline + Galactose	Flexible with balloon (6 Fr)	5	Vaginal	2D	Yes	No	Yes
Dijkman <i>et al.</i> (2000)	100	200 (106)	Netherlands	English	Subfertility	0.28	Saline + Galactose	Flexible with balloon	7.5	Vaginal	2D	No	Yes	Yes
Friberg and Joergense (1994)	14	28 (10)	Sweden	English	Subfertility with planned laparoscopy	0.50	Saline	Flexible with balloon	6.5	Vaginal	2D	No	No	Yes
Guerriero <i>et al.</i> (1996)	30	60 (0)	Italy	English	Subfertility	0.30	Galactose	Flexible with balloon (5 Fr)	5	Vaginal	2D	Yes	No	Yes
Hauge <i>et al.</i> (2000)	33	66 (0)	Norway	English	Subfertility with planned laparoscopy	0.21	Saline + Galactose	Flexible with balloon (4 Fr)	7.5	Vaginal	2D	No	No	Yes
Heikkinen <i>et al.</i> (1995)	31	61 (0)	Finland and Italy	English	Subfertility	0.18	Saline + air	Flexible with balloon (6–10 Fr)	5–6.5	Vaginal	2D	Yes	No	Yes
Inki <i>et al.</i> (1998)	32	53 (11)	Finland	English	Subfertility	0.23	Saline + air	Flexible with balloon (6 Fr)	6	Vaginal	2D	No	No	Yes
Kozarzewski <i>et al.</i> (1995)	25	50 (0)	Poland	Polish	Subfertility	0.20	Galactose	Rigid	3.75	Abdominal	2D	Yes	Yes	Yes
Kupescic and Plavsic (2007)	268	536 (0)	Croatia	English	Subfertility (91%) and RPL (9%)	0.46	Galactose	Flexible with balloon (5 Fr)	5–7	Vaginal	2D 3D	Yes	No	Yes

Continued

Table I Continued

Studies	Participants	Tubes ^a (excluded)	Country	Language	Population	Prevalence ^b	Contrast	Catheter	Resolution (MHz)	Probe	2D or 3D	Doppler	Comparison with HSG ²	In MA
Luciano et al. (2011)	62	121 (0)	USA	English	Subfertility with planned laparoscopy	0.41	Saline + air	Flexible with balloon (5 Fr)	5–9	Vaginal	2D	No	No	Yes
Omigbodun et al. (1992)	31	62 (6)	Nigeria	English	Subfertility	0.36	Saline	Rigid	3.5	Abdominal	2D	No	No	Yes
Radic et al. (2005)	68	135 (0)	Croatia	English	Subfertility (66%) and RPL (34%)	0.35	Saline + Galactose	Flexible with balloon (8 Fr)	6.5	Vaginal	2D	No	No	Yes
Randolph et al. (1986)	61	122 (2)	United States	English	Subfertility and RPL	0.07	Saline	Rigid	3.5	Abdominal	2D	No	Yes	No
Reis et al. (1998)	44	88 (0)	Brazil	English	Subfertility	0.31	Saline + Galactose	Flexible with balloon (6 Fr)	—	Vaginal	2D	No	Yes	Yes
Schwarzler et al. (1997)	57	108 (0)	Austria	German	Subfertility	0.22	—	(6 Fr)	7.5	Vaginal	2D	Yes	No	Yes
Socolov et al. (2009)	95	181 (0)	Romania	Romanian	Subfertility	0.36	Saline + air	Flexible with balloon	7	Vaginal	3D	No	Yes	Yes
Spalding et al. (1997)	32	59 (4)	Finland	English	Subfertility with planned laparoscopy	0.22	Saline + air or Galactose	Flexible with balloon	6	Vaginal	2D	No	No	Yes
Tanawattanacharoen et al. (1998)	15	25 (5)	Thailand	English	Subfertility	0.36	Galactose	?	5	Vaginal	2D	Yes	No	Yes
Tufekci et al. (1992)	44	88 (16)	Turkey	English	Subfertility	0.28	Saline	Flexible with balloon (8 Fr)	5	Vaginal	2D	No	No	Yes
Wang et al. (2012)	70	140 (0)	China	Mandarin	Subfertility	0.46	SonoVue	?	9	Vaginal	2D			
Watermann et al. (2004)	21	42 (0)	Germany	German	Subfertility with planned laparoscopy	0.12	Galactose	Flexible with balloon (5 Fr)	5–8	Vaginal	3D	No	No	Yes

2D, two-dimensional; 3D, three-dimensional; Fr, French; MA, meta-analysis; RPL, recurrent pregnancy loss.

^aNumber of tubes may not be consistent with the number of patients because of past salpingectomy and unicornuate uterus. In parenthesis is the number of tubes excluded from the analyses for each study. The reasons reported for exclusions were: poor visualisation, cervical stenosis, pain, suspicion of hydrosalpinx at sonography (sono-HSG cancelled), pregnancy and the women failed to return for the other test.

^bPrevalence of tubal occlusion per tube.

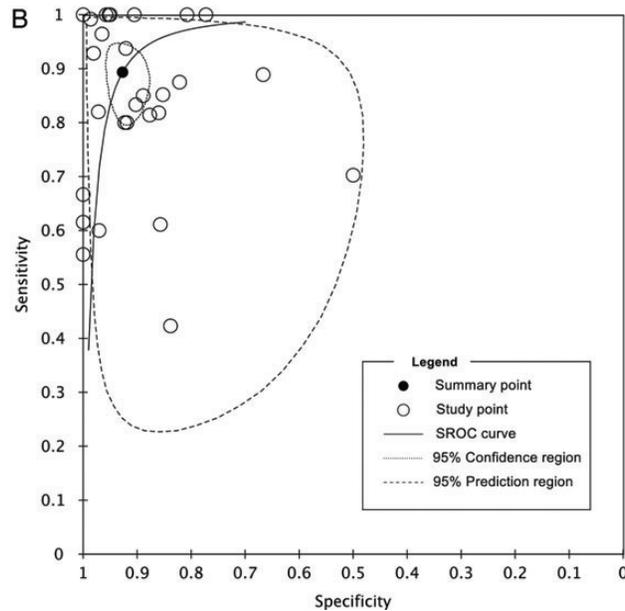
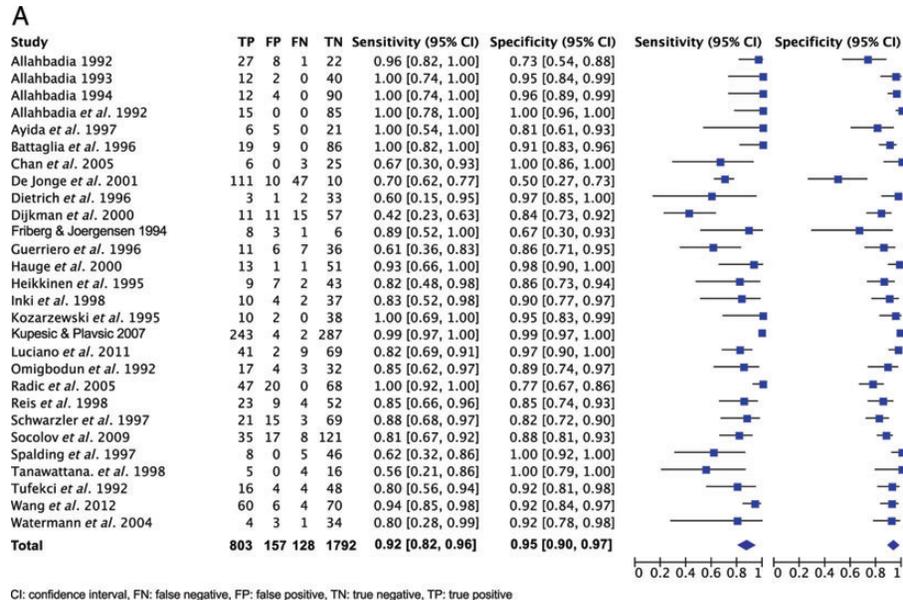


Figure 2 (A) Forest plot of sono-HSG and (B) summary ROCs (SROC) curve for diagnosing tubal occlusion (per tube).

fever 0.8%). Patient tolerance of sono-HSG was compared with HSG in a RCT (Ayida et al., 1996) and no difference in pain, need for analgesia or side-effects was observed at 2 h, 24 h and 28 days after the procedure. There was also no significant difference in terms of procedure duration.

The costs of sono-HSG and HSG can vary but are nonetheless considered similar (Lim et al., 2011). However, sono-HSG could be considered as more cost-effective since it allows a complete assessment of the pelvis. Some authors argue that a complete pelvic ultrasound scan should be part of the evaluation of subfertile women as it provides useful information for treatment decisions and prognosis (Kelly et al., 2001). In fact, complete assessment of the uterus, uterine cavity, endometrium, ovaries, follicles, tubes and their patency could detect relevant anomalies

that would otherwise result in prolonged, invasive or unnecessary interventions (Kelly et al., 2001).

We observed heterogeneity of our results, which is to be expected in diagnostic test accuracy reviews (Macaskill et al., 2010). Some between-study heterogeneity could be due to differences in study populations (e.g. BMI, pain tolerance) and in provider expertise (Exacoustos et al., 2009). Subgroup analyses showed that heterogeneity is partly explained by variations in the sono-HSG technique. Doppler sonography leads to coloration of fluid flow through the tubes and was associated in our review with significantly greater sensitivity and specificity of sono-HSG. Spilling of contrast from the fimbrial end of the tube is difficult to distinguish from the bowel, both of them having similar echogenicity (Sladkevicius

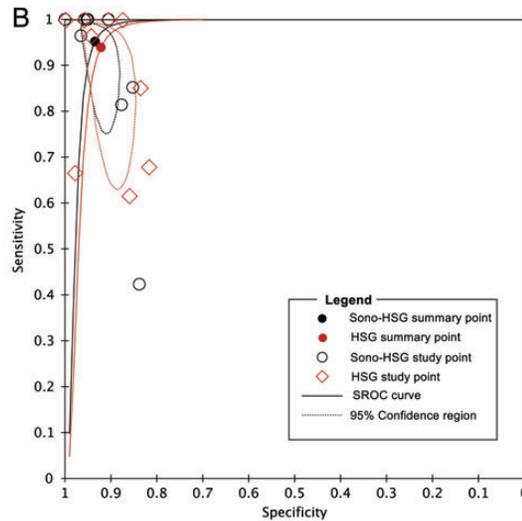
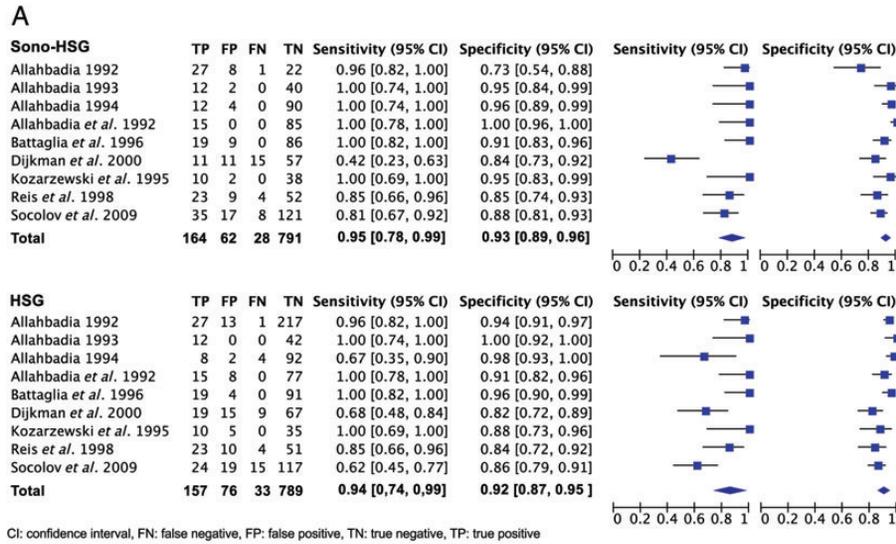


Figure 3 (A) Forest plot and (B) summaries (SROC) from direct comparison of sono-HSG and HSG for diagnosing tubal occlusion (per tube) (P -value based on likelihood ratio χ^2 statistic = 0.04).

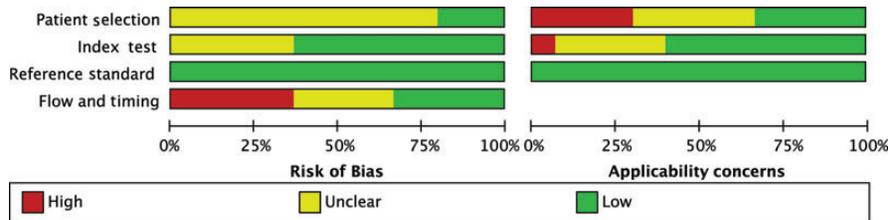


Figure 4 Risk of bias and applicability concerns based on QUADAS-2 presented as percentages across included studies.

et al., 2000). The benefits of Doppler sonography could be explained by its capacity to enhance the visualization of fluid flow from tubes to the pelvis (Sladkevicius et al., 2000).

Hyperechogenic contrast media, e.g. Echovist-200 (Schering AG, Berlin, Germany), ExEm-gel foam (GynaecologiQ, Delft, The

Netherlands) and SonoVue (Bracco, Milan, Italy), have been commercialized to facilitate the liquid visualization in the tubes (Exacoustos et al., 2009). In our review, we found no benefit of these contrast media over saline solution in regard to the diagnostic accuracy of sono-HSG. Saline solution mixed with air also has a hyperechoic appearance

Table II Subgroup and sensitivity analyses.

Variables	Number of studies ^a	Number of women	Number of tubes	Sensitivity (95% CI)	Specificity (95% CI)	P
Doppler						
Yes	13	785	1545	0.93 (0.84–0.97)	0.95 (0.92–0.98)	0.0497
No	15	766	1335	0.86 (0.74–0.93)	0.89 (0.83–0.93)	
2D or 3D						
3D	5	293	641	0.89 (0.77–0.95)	0.94 (0.86–0.98)	0.6703
2D	26	1258	2281	0.88 (0.80–0.94)	0.92 (0.87–0.95)	
Contrast						
Saline	14	643	1223	0.91 (0.82–0.96)	0.93 (0.88–0.96)	
Other contrasts	16	851	1657	0.87 (0.76–0.94)	0.92 (0.86–0.96)	0.7046
Risk of bias ^b						
High	15	952	1701	0.88 (0.77–0.94)	0.91 (0.85–0.95)	
Low/unclear	13	599	1179	0.91 (0.80–0.96)	0.94 (0.89–0.97)	0.5488

^aStudies that reported several techniques were retained in subgroup analyses if they provided data separately for each technique. For this reason, some studies may be counted more than once in each analysis.

^bGlobal appreciation for risk of bias and applicability concerns based on the QUADAS-2. CI, confidence interval; 2D, two-dimensional; 3D, three-dimensional.

(Exacoustos *et al.*, 2009). In addition, saline is safe, has no risk of allergy, and is far less expensive than commercial contrast media (Exacoustos *et al.*, 2009). This economical aspect further enhances the advantages of using sono-HSG over HSG.

We observed no significant increase in the diagnostic accuracy of sono-HSG with a 3D device. However, 3D has other benefits compared with 2D that must be considered, namely, it requires less time (Sladkevicius *et al.*, 2000), avoids difficult probe movements and is less dependent on operator skill (Exacoustos *et al.*, 2009). Image acquisition also permits storage and later analyses of captures (Exacoustos *et al.*, 2009).

Our systematic review has some strengths and limitations. First, laparoscopy with chromotubation is largely accepted as the gold standard for diagnosing tubal occlusion (Mol *et al.*, 1999; Saunders *et al.*, 2011; NICE, 2013) as its findings are highly correlated with spontaneous pregnancy rates (Mol *et al.*, 1999), but still diagnostic errors can occur with technical problems (e.g. improper catheter placement, lack of sealing) or severe adhesions (Saunders *et al.*, 2011). In some studies, tubes could not be assessed by either sono-HSG or laparoscopy given a lack of visualization. Such exclusions from the analysis may have affected the validity of the results of the concerned studies. Also, applicability concerns were raised in 2 of the 30 included studies that did not only consider subfertile women, but also women suffering from recurrent pregnancy losses. These aspects were taken into account in the assessment of risk bias and applicability concerns using the QUADAS-2 tool. In a sensitivity analysis, the pooled estimates of sensitivity and specificity of sono-HSG did not significantly differ for the 15 studies that were attributed at least one high risk of bias or applicability concern compared with the other studies included in our systematic review. In other words, the variation in the methodological quality of the included studies did not significantly modify the results of our pooled estimates.

In 28 of the 30 included studies, results were reported per tube, not per woman, which allowed us to calculate pooled estimate per tube. Reporting the results per woman brings the problem of multiple possible definitions of a positive test (both tubes occluded or at least on tube

occluded) and, thereby, different values of sensitivity and specificity (Broeze *et al.*, 2012). However, the data for each tube of a woman are not independent. In our analyses, we have not been able to account for this cluster effect, as the results reported for each individual study did not allow us to link tubes together in regards to their belonging to a single woman. To ignore the cluster effect has no effect on the point estimates of sensitivity and specificity but can affect the width of the 95% CI; however, given the high number of women (cluster), the estimates were probably hardly affected. Finally, this systematic review did not allow the distinction between distal and proximal occlusion. This could be interesting to take into account in further studies as the performance of the test may differ for each localization.

Direct comparison of sono-HSG and HSG (all tests performed on all participants) reduced the possibility of confounding biases and increased the validity of our results (Macaskill *et al.*, 2010). Our searches were extensive in different databases. We applied no restrictions based on language and did not systematically exclude studies with partial verification bias, enhancing the validity, precision and generalizability of our results (Irwig *et al.*, 1994; de Groot *et al.*, 2011; de Groot *et al.*, 2012). Finally, important strengths of our review lay in the *a priori* nature of our protocol (Maheux-Lacroix *et al.*, 2013) and methods adhering to recent guidelines for diagnostic test accuracy reviews (de Vet *et al.*, 2008; Liberati *et al.*, 2009; Macaskill *et al.*, 2010; Whiting *et al.*, 2011; Reitsma *et al.*, 2012).

In conclusion, sono-HSG is an accurate test for diagnosing tubal occlusion and performs similarly to HSG. Given their comparable patient tolerability and the advantages of sono-HSG over HSG (visualization of ovaries and myometrium, better sensitivity and specificity for the diagnosis of uterine cavity abnormalities, absence of radiation and risk of iodine allergy), sono-HSG should replace HSG in the initial workup of subfertile couples. An economic study comparing cost-utility of sono-HSG and HSG would add an interesting perspective to these considerations. Finally, Doppler sonography potentially improves the diagnostic accuracy of sono-HSG and deserves further evaluation.

Authors' roles

S.M.-L. was involved in data collection, statistical analysis, manuscript preparation and revision, construction of figures and tables and submission of manuscript. A.B. was involved in data collection. L.M. served as advisor on analytical methods. A.B., L.M., M.-E.B., E.B., P.L., M.L., S.D. were involved in interpreting the data, as well as writing and revising manuscript.

Funding

This study was funded by personal funds. S.M.-L. is recipient of a PhD award from the Fonds de Recherche Québec-Santé. L.M. is recipient of a New Investigator Awards from the Canadian Institute of Health Research (CIHR). E.B. hold a Clinician Scientist Award from the CIHR and the Jeanne et Jean-Louis Lévesque Research Chair at Université Laval. A.B. is recipient of a PhD Award from CIHR.

Conflict of interest

None of the authors have conflicts of interest to declare.

References

- Acholonu UC, Silberzweig J, Stein DE, Keltz M. Hysterosalpingography versus sonohysterography for intrauterine abnormalities. *JLSLS* 2011; **15**:471–474.
- Allahbadia G. Fallopian tubes and ultrasonography: the Sion experience. *Fertil Steril* 1992; **58**:901–907.
- Allahbadia GN. Fallopian tube patency using color Doppler. *Int J Gynaecol Obstet* 1993; **40**:241–244.
- Allahbadia GN. Colour-coded duplex sonography for the assessment of fallopian tube patency. *Ann Acad Med Singapore* 1994; **23**:98–101.
- Allahbadia GN, Nalawade YV, Patkar VD, Niyogi GM, Shah PK. The Sion test. *Aust N Z J Obstet Gynaecol* 1992; **32**:67–70.
- Ayida G, Kennedy S, Barlow D, Chamberlain P. A comparison of patient tolerance of hysterosalpingo-contrast sonography (HyCoSy) with Echovist-200 and X-ray hysterosalpingography for outpatient investigation of infertile women. *Ultrasound Obstet Gynecol* 1996; **7**:201–204.
- Ayida G, Chamberlain P, Barlow D, Koninckx P, Golding S, Kennedy S. Is routine diagnostic laparoscopy for infertility still justified? A pilot study assessing the use of hysterosalpingo-contrast sonography and magnetic resonance imaging. *Hum Reprod* 1997; **12**:1436–1439.
- Battaglia C, Artini PG, D'Ambrogio G, Genazzani AD, Genazzani AR, Volpe A. Color Doppler hysterosalpingography in the diagnosis of tubal patency. *Fertil Steril* 1996; **65**:317–322.
- Broeze KA, Opmeer BC, Coppus SF, Van Geloven N, Den Hartog JE, Land JA, Van der Linden PJ, Ng EH, Van der Steeg JW, Steures P et al. Integration of patient characteristics and the results of Chlamydia antibody testing and hysterosalpingography in the diagnosis of tubal pathology: an individual patient data meta-analysis. *Hum Reprod* 2012; **27**:2979–2990.
- Chan CC, Ng EH, Tang OS, Chan KK, Ho PC. Comparison of three-dimensional hysterosalpingo-contrast-sonography and diagnostic laparoscopy with chromopertubation in the assessment of tubal patency for the investigation of subfertility. *Acta Obstet Gynecol Scand* 2005; **84**:909–913.
- de Almeida I, Souza C, Reginatto F, Cunha Filho JS, Facin A, Freitas F, Lavic Y, Passos EP. [Hysterosonosalingography and hysterosalpingography in the diagnosis of tubal patency in infertility patients]. *Rev Assoc Med Bras* 2000; **46**:342–345.
- de Groot JA, Dendukuri N, Janssen KJ, Reitsma JB, Bossuyt PM, Moons KG. Adjusting for differential-verification bias in diagnostic-accuracy studies: a Bayesian approach. *Epidemiol* 2011; **22**:234–241.
- de Groot JA, Dendukuri N, Janssen KJ, Reitsma JB, Brophy J, Joseph L, Bossuyt PM, Moons KG. Adjusting for partial verification or workup bias in meta-analyses of diagnostic accuracy studies. *Am J Epidemiol* 2012; **175**:847–853.
- De Jonge ETM, Hartman CR, Swaenepoel HM, Pistorius LR, Ombelet W. Hysterosalpingo-contrast-sonography as a triage for tubal patency in a population at risk for pelvic infection. *Middle East Fertil Soc J* 2001; **6**:239–244.
- de Vet H, Eisinga A, Riphagen I, Aertgeerts B, Pewsner D, Mitchell R. Chapter 7: searching for studies. In: Deeks JJ, Bossuyt PM, Gatsonis C (eds). *Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy Version 1.0.0*. The Cochrane Collaboration, 2008. Available from: srdta.cochrane.org.
- Deeks J, Bossuyt P, Gatsonis C. *Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy Version 1.0.0*. Cochrane Collaboration, 2008. Available from: srdta.cochrane.org.
- Dessole S, Farina M, Rubattu G, Cosmi E, Ambrosini G, Battista Nardelli G. Side effects and complications of sonohysterosalpingography. *Fertil Steril* 2003; **80**:620.
- Dietrich M, Suren A, Hinney B, Osmers R, Kuhn W. Evaluation of tubal patency by hysterocontrast sonography (HyCoSy, Echovist) and its correlation with laparoscopic findings. *J Clin Ultrasound* 1996; **24**:523–527.
- Dijkman AB, Mol BW, van der Veen F, Bossuyt PM, Hogerzeil HV. Can hysterosalpingocontrast-sonography replace hysterosalpingography in the assessment of tubal subfertility? *Eur J Radiol* 2000; **35**:44–48.
- Exacoustos C, Di Giovanni A, Szabolcs B, Binder-Reisinger H, Gabardi C, Arduini D. Automated sonographic tubal patency evaluation with three-dimensional coded contrast imaging (CCI) during hysterosalpingo-contrast sonography (HyCoSy). *Ultrasound Obstet Gynecol* 2009; **34**:609–612.
- Friberg B, Joergensen C. Tubal patency studied by ultrasonography. A pilot study. *Acta Obstet Gynecol Scand* 1994; **73**:53–55.
- Guerrero S, Ajossa S, Mais V, Paoletti AM, Melis GB. The screening of tubal abnormalities in the infertile couple. *J Assist Reprod Genet* 1996; **13**:407–412.
- Hauge K, Flo K, Riedhart M, Granberg S. Can ultrasound-based investigations replace laparoscopy and hysteroscopy in infertility? *Eur J Obstet Gynecol Reprod Biol* 2000; **92**:167–170.
- Heikkinen H, Tekay A, Volpi E, Martikainen H, Jouppila P. Transvaginal salpingosonography for the assessment of tubal patency in infertile women: methodological and clinical experiences. *Fertil Steril* 1995; **64**:293–298.
- Holz K, Becker R, Schürmann R. Ultrasound in the investigation of tubal patency. A meta-analysis of three comparative studies of Echovist-200 including 1007 women. *Zentralbl Gynakol* 1997; **119**:366.
- Inki P, Palo P, Anttila L. Vaginal sonosalpingography in the evaluation of tubal patency. *Acta Obstet Gynecol Scand* 1998; **77**:978–982.
- Irwig L, Tosteson ANA, Gatsonis C, Lau J, Colditz G, Chalmers TC, Mosteller F. Guidelines for meta-analyses evaluating diagnostic tests. *Ann Intern Med* 1994; **120**:667–676.
- Kelly SM, Sladkevicius P, Campbell S, Nargund G. Investigation of the infertile couple: a one-stop ultrasound-based approach. *Hum Reprod* 2001; **16**:2481–2484.
- Kiyokawa K, Masuda H, Fuyuki T, Koseki M, Uchida N, Fukuda T, Amemiya K, Shouka K, Suzuki K. Three-dimensional hysterosalpingo-contrast sonography (3D-HyCoSy) as an outpatient procedure to assess infertile women: a pilot study. *Ultrasound Obstet Gynecol* 2000; **16**:648–654.
- Kozarzewski M, Szaflik K, Pertynski T, Banaszczuk R, Radwan J. [Evaluation of the value of clinical doppler sonography and sonographic contrast media for assessment of tubal patency]. *Ginekol Pol* 1995; **66**:633–637.

- Kupesic S, Plavsic BM. 2D and 3D hysterosalpingo-contrast-sonography in the assessment of uterine cavity and tubal patency. *Eur J Obstet Gynecol Reprod Biol* 2007;**133**:64–69.
- Leefflang MM, Scholten RJ, Rutjes AWW, Reitsma JB, Bossuyt PM. Use of methodological search filters to identify diagnostic accuracy studies can lead to the omission of relevant studies. *J Clin Epidemiol* 2006;**59**:234–240.
- Liberati A, Altman DG, Tetzlaff J, Mulrow C, Gotzsche PC, Ioannidis JP, Clarke M, Devereaux PJ, Kleijnen J, Moher D. The PRISMA statement for reporting systematic reviews and meta-analyses of studies that evaluate healthcare interventions: explanation and elaboration. *Br Med J* 2009;**339**:b2700.
- Lim CP, Hasafa Z, Bhattacharya S, Maheshwari A. Should a hysterosalpingogram be a first-line investigation to diagnose female tubal subfertility in the modern subfertility workup? *Hum Reprod* 2011;**26**:967–971.
- Luciano DE, Exacoustos C, Johns A, Luciano AA. Can hysterosalpingo-contrast sonography replace hysterosalpingography in confirming tubal blockage after hysteroscopic sterilization and in the evaluation of the uterus and tubes in infertile patients? *Am J Obstet Gynecol* 2011;**204**:Article No.: 79.e71.
- Macaskill P, Gatsonis C, Deeks JJ, Harbord RM, Takwoingi Y. Chapter 10: analysing and presenting results. In: Deeks JJ, Bossuyt PM, Gatsonis C (eds). *Cochrane Handbook for Systematic Reviews of Diagnostic Test Accuracy Version 1.0*. The Cochrane Collaboration, 2010. Available from: <http://srdta.cochrane.org/>.
- Maheux-Lacroix S, Boutin A, Moore L, Bergeron M, Bujold E, Laberge P, Lemyre M, Dodin S. Hysterosalpingosonography for diagnosing tubal occlusion in subfertile women: a systematic review protocol. *Syst Rev* 2013;**2**:50.
- Mol B, Collins J, Burrows E, van der Veen F, Bossuyt P. Comparison of hysterosalpingography and laparoscopy in predicting fertility outcome. *Hum Reprod* 1999;**14**:1237–1242.
- NICE: National Institute for Health and Clinical Excellence. *Fertility: Assessment and Treatment for People with Fertility Problems*. NICE clinical guideline 156, 2013. www.guidance.net.org.uk/cg156.
- Omigbodun AO, Fatukasi JJ, Abudu T. Ultrasonography as an adjunct to hydrotubation in the management of female infertility. *Cent Afr J Med* 1992;**38**:345–350.
- Radic V, Canic T, Valetic J, Ducic Z. Advantages and disadvantages of hysterosalpingography in the assessment of the reproductive status of uterine cavity and fallopian tubes. *Eur J Radiol* 2005;**53**:268–273.
- Randolph JF, Ying YK, Maier DB, Schmidt CL, Riddick DH. Comparison of real-time ultrasonography, hysterosalpingography, and laparoscopy/hysteroscopy in the evaluation of uterine abnormalities and tubal patency. *Fertil Steril* 1986;**46**:828–832.
- Reis MM, Soares SR, Cancado ML, Camargos AF. Hysterosalpingo contrast sonography (HyCoSy) with SH U 454 (Echovist) for the assessment of tubal patency. *Hum Reprod* 1998;**13**:3049–3052.
- Reitsma JB, Moons KG, Bossuyt PM, Linnet K. Systematic reviews of studies quantifying the accuracy of diagnostic tests and markers. *Clin Chem* 2012;**58**:1534–1545.
- Sankpal RS, Confino E, Matzel A, Cohen LS. Investigation of the uterine cavity and fallopian tubes using three-dimensional saline sonohysterosalpingography. *Int J Gynecol Obstet* 2001;**73**:125–129.
- Saunders RD, Shwayder JM, Nakajima ST. Current methods of tubal patency assessment. *Fertil Steril* 2011;**95**:2171–2179.
- Savelli L, Pollastri P, Guerrini M, Villa G, Manuzzi L, Mabrouk M, Rossi S, Seracchioli R. Tolerability, side effects, and complications of hysterosalpingocontrast sonography (HyCoSy). *Fertil Steril* 2009;**92**:1481–1486.
- Schwarzler P, Concin H, Wohlgenannt K. [Cost effective media in vaginal ultrasound uterus and fallopian tube diagnosis]. *Ultraschall Med* 1997;**18**:8–13.
- Sladkevicius P, Ojha K, Campbell S, Nargund G. Three-dimensional power Doppler imaging in the assessment of Fallopian tube patency. *Ultrasound Obstet Gynecol* 2000;**16**:644–647.
- Soares SR, dos Reis MMB, Camargos AF. Diagnostic accuracy of sonohysteroscopy, transvaginal sonography, and hysterosalpingography in patients with uterine cavity diseases. *Fertil Steril* 2000;**73**:406–411.
- Socolov D, Lupascu IA, Danciu E, Doroftei B, Boian I, Boiculescu L, Pintilie P, Miron N. [Sonohysterosalpingography versus hysterosalpingography in the evaluation of uterine and tubal infertility]. *Rev Med Chir Soc Med Nat Iasi* 2009;**113**:803–808.
- Socolov D, Boian I, Boiculescu L, Tamba B, Anghelache-Lupascu I, Socolov R. Comparison of the pain experienced by infertile women undergoing hysterosalpingo contrast sonography or radiographic hysterosalpingography. *Int J Gynecol Obstet* 2010;**111**:256–259.
- Spalding H, Martikainen H, Tekay A, Jouppila P. A randomized study comparing air to Echovist (registered trademark) as a contrast medium in the assessment of tubal patency in infertile women using transvaginal salpingosonography. *Hum Reprod* 1997;**12**:2461–2464.
- Tanawattanacharoen S, Suwajanakorn S, Uerpairojkit B, Wisawasukmongchol W, Boonkasemsanti W, Virutamasen P. Transvaginal hysterosalpingo-contrast sonography (HyCoSy) compared with chromolaparoscopy: a preliminary report. *J Med Assoc Thai* 1998;**81**:520–526.
- Tufekci EC, Girit S, Bayirli E, Durmusoglu F, Yalti S. Evaluation of tubal patency by transvaginal sonosalpingography. *Fertil Steril* 1992;**57**:336–340.
- Wang Y, Zhang Y, Qu X, She Y. A comparison between 3D coded contrast imaging and 2D hysterosalpingo-contrast-sonography. *J. China Med. Univ.* 2012;**41**:650.
- Watermann D, Denschlag D, Hanjalic-Beck A, Keck C, Karck U, Prompeler H. [Hystero-salpingo-contrast-sonography with 3-d-ultrasound—a pilot study]. *Ultraschall Med* 2004;**25**:367–372.
- Whiting PF, Rutjes AWW, Westwood ME, Mallett S, Deeks JJ, Reitsma JB, Leeflang MM, Sterne JA, Bossuyt PM. QUADAS-2: a revised tool for the quality assessment of diagnostic accuracy studies. *Ann Intern Med* 2011;**155**:529–536.